


RAYCAST® HIGH PRECISION BASE PLATE IN CARBON FIBRE LAMINATE – EXTENDED VERSION

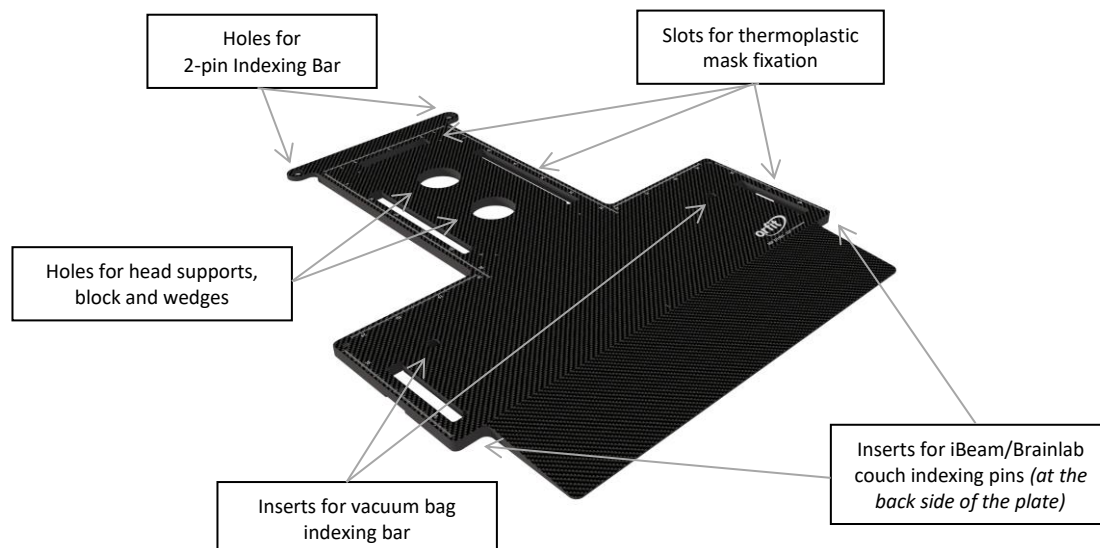

Article No. : **32110/12**

A. GENERAL PRODUCT INFORMATION

This product is a medical device used for patient positioning and immobilisation (head & neck) in radiation therapy. This low density plate can be used during both the simulation and the treatment stage.

This product may only be used in combination with immobilisation masks produced by Orfit. Orfit prohibits the use of unauthorized third-party products in conjunction with its own products

B. PRODUCT DESCRIPTION

This RAYCAST® HIGH PRECISION BASE PLATE – EXTENDED VERSION in Carbon Fibre Laminate (CFL) is suitable for use in combination with the range of Efficast® thermoplastic Head & Neck and Head, Neck & Shoulders masks, Raycast® High Precision Head Supports, Blocks, Wedges and Couch Indexing Devices to form a reproducible patient positioning and immobilisation device in the field of radiotherapy. Information on these other parts and instructions on how to make the masks can be found in the respective 'instructions for use' and on www.orfit.com.

The base plate has an extended and chamfered edge to avoid the creation of pressure points in the back of the patient.

C. PRECAUTIONS FOR USE

Always place the base plate on a flat surface and make sure that it is completely supported by the couch.

Always fix the base plate securely to the treatment couch before positioning a patient. More information on how to fix this base plate to a couch top can be found on our website <http://www.orfit.com/en/fixation-devices/>.

The CFL base plate is constructed to be light in weight and to have superb dosimetric properties. When handled roughly, it may get damaged and fibres may come off. When this happens, stop using the base plate to prevent fibres from getting in contact with the patient's or user's skin. Contact your distributor.

A patient set-up form is available on the Orfit website: <https://www.orfit.com/app/uploads/Head-and-Neck.pdf>

D. STORAGE

Always store the product in a safe place to prevent it from getting damaged or falling onto other objects. Take care not to damage the edges of the plate when storing it in an upright position. Prevent hard objects from falling onto the plate. Store the base plate between +10°C (50°F) and 40°C (122°F).

E. PROPERTIES


E.1 Physical Properties

This plate is made of a carbon fibre laminate.

Dimensions: L 627 mm x W 540 mm x H 12 mm
L 24.69" x W 21.26" x 0.47"
Weight : 0.79 kg
1.74 lbs

E.2 Dosimetric Properties

Position	Attenuation (± 0.15 %) (6MV)	Attenuation (± 0.15 %) (15MV)	Skin build-up (± 0.1 mm) (15MV)
	%	%	mm H ₂ O equiv.
1	1.09	0.60	3.17
2	1.07	0.55	2.94
3	1.65	0.97	4.79
4	0.77	0.34	2.01

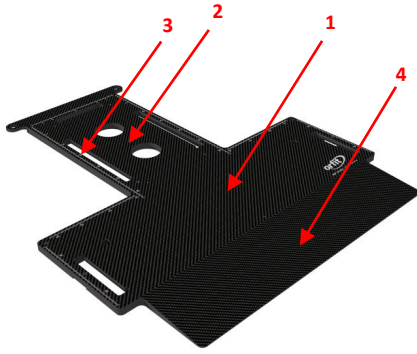

Note: Use these numbers as a guidance only. Perform the measurements again in your department to verify these results.

F. MAINTENANCE AND WASTE MANAGEMENT

This product can be cleaned and disinfected by means of an isopropanol based disinfectant, applied with a soft cloth. If unsure about the cleaning fluid, do not use. **Never use aerosol sprays, corrosive cleaning agents, solvents or abrasive detergents.**

Periodic checks of the product should be done to insure the parts are not worn and require repair or replacement. **Do not attempt to make repairs yourself.** Contact your distributor if there are any questions or concerns. The product can be disposed of with household waste.

G. PACKAGES

This product is part of following packages:

- 36401: SRS-Fix Hardware Starter Package 1
- 36402: SRS-Fix Hardware Starter Package 2

H. ADDITIONAL INFORMATION

For additional information such as distributor contact information, product brochures, Safety Data Sheets and regulatory information, please visit our website www.orfit.com.

Note:

It is prohibited to make alterations to this text without prior approval from Orfit Industries. RAYCAST® and EFFICAST® are registered trademarks of Orfit Industries.



ORFIT INDUSTRIES
Vosveld 9A | B-2110 Wijnegem | Belgium
T (+32) (0)3 326 20 26
welcome@orfit.com

www.orfit.com



Ref. No. 50175
VERSION 2
LAST UPDATE: 13/04/2021
REVISION DATE: 13/04/2023